



Overall Performance

Survey Contents:

Specimen 1: **1701DL1** Matrix DA for 5 Population Instruments

Specimen 2: **1701DL2** Matrix DA for 5 Population Instruments








Non Participation Penalty: 0

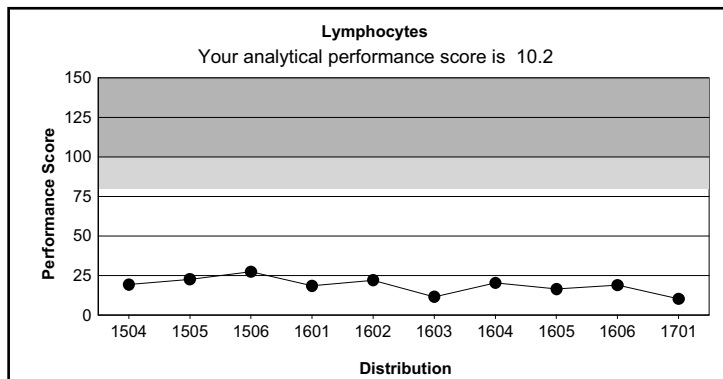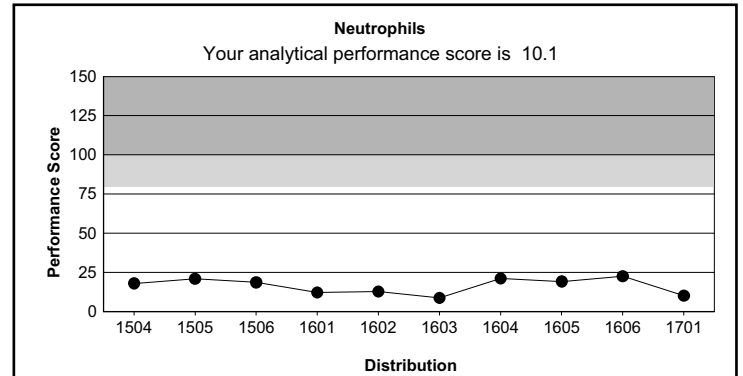

This report shows information for the instruments which used **Matrix DA**.
The specimens for Matrix DA 1701DL1 & 1701DL2 were suitable for 5
population instruments from the following manufacturers: Siemens

■ Your Method

Sample Quality
You reported : Satisfactory
Overall
Satisfactory % : 99.5
Unsatisfactory % : 0.5

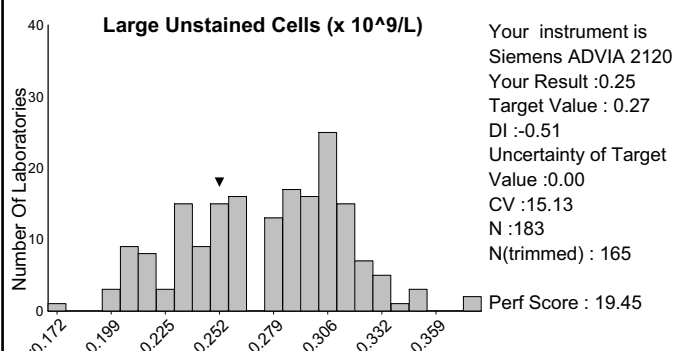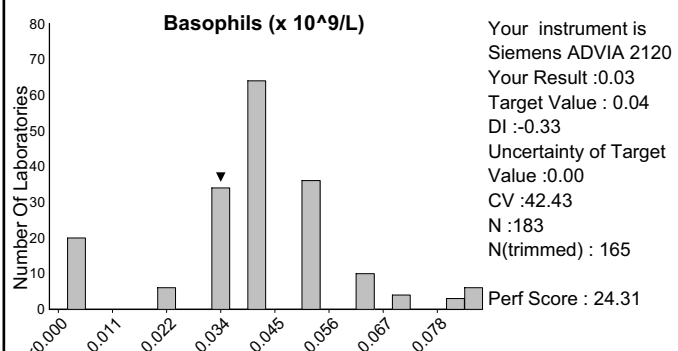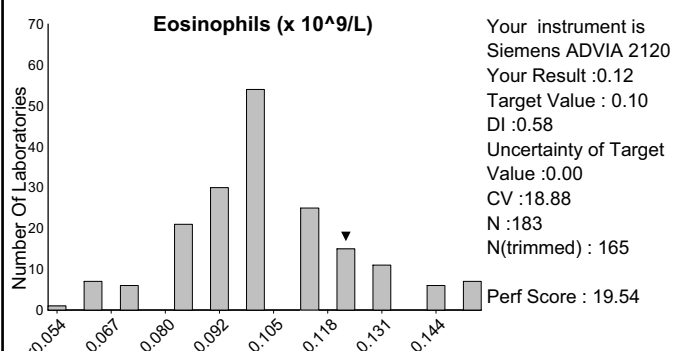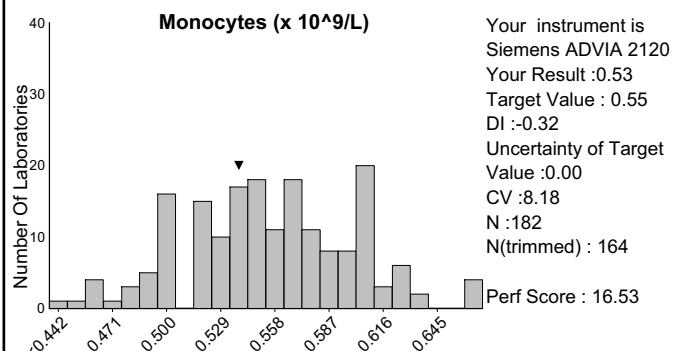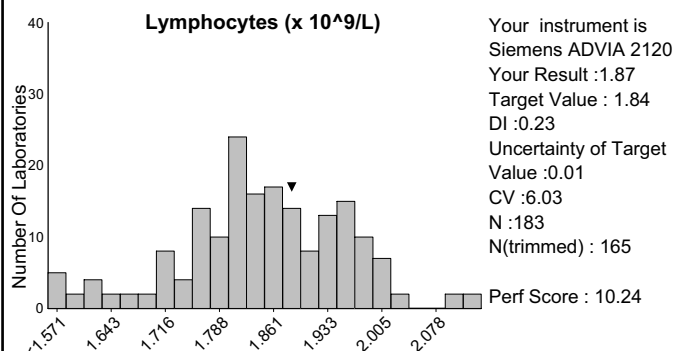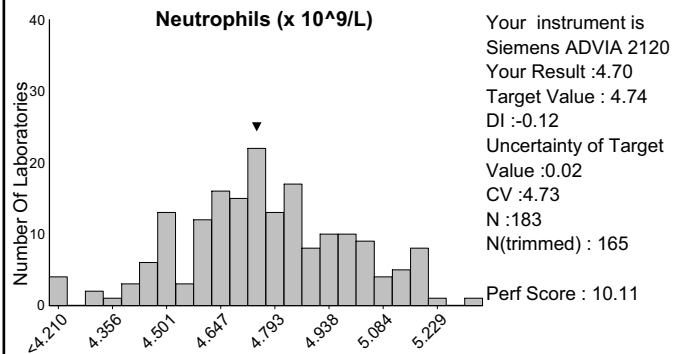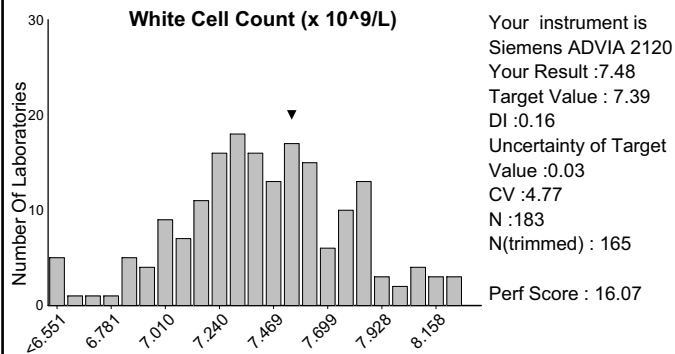

This report shows information for the instruments which used **Matrix DA**.
The specimens for Matrix DA 1701DL1 & 1701DL2 were suitable for 5
population instruments from the following manufacturers: Siemens

■ Your Method

Sample Quality
You reported : Satisfactory
Overall
Satisfactory % : 99.2
Unsatisfactory % : 0.8

