
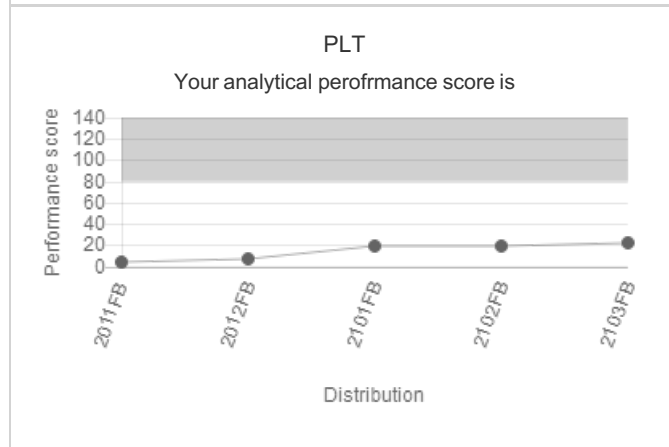
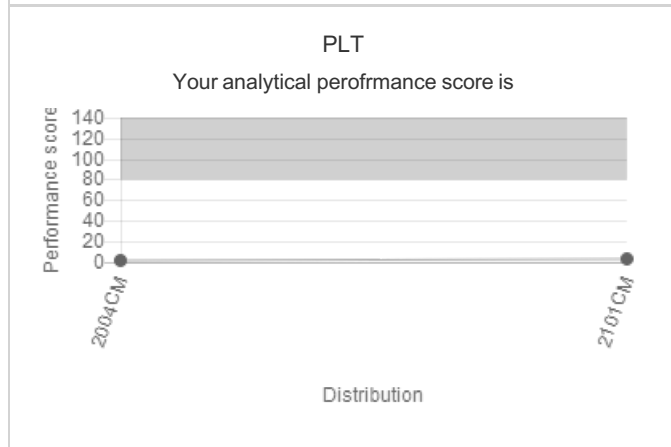
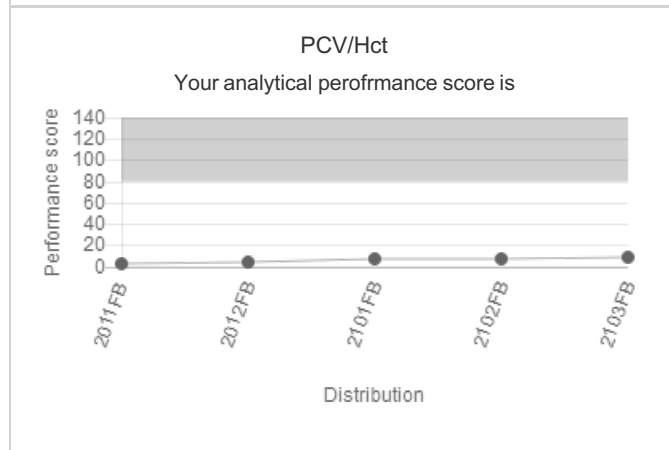
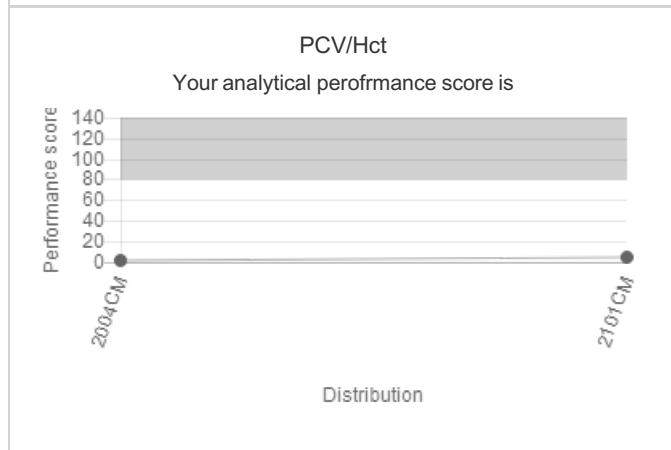
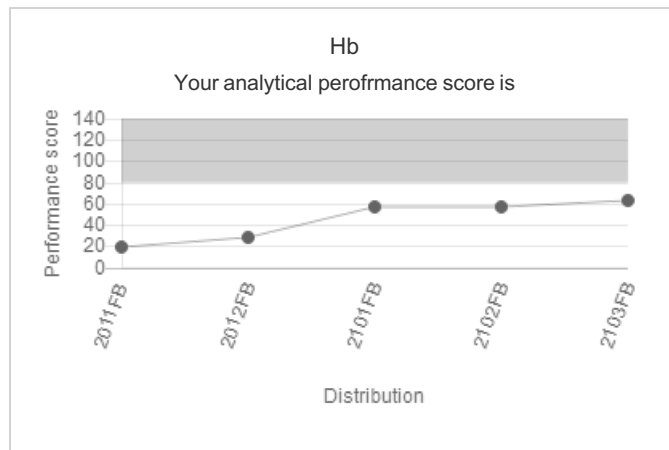


Overall performance

Blood Component Monitoring

Full Blood Count (for comparison)

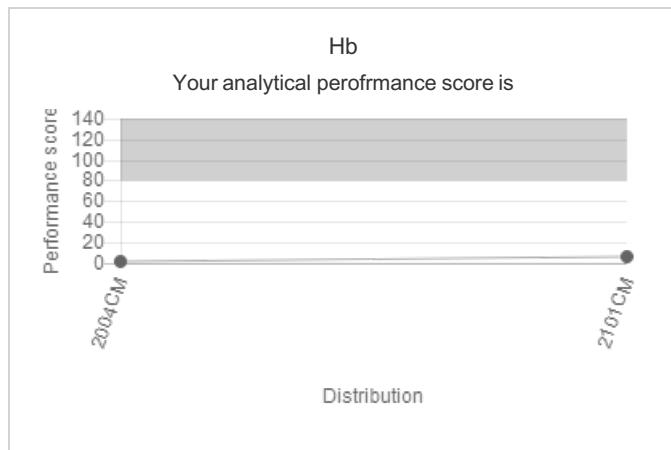

Printed at 9:25 on Thursday, 17 June, 2021 (Final Report)

For information on data analysis and performance assessment see the [UK NEQAS Haematology Participant's Manual](#)

Scheme Director: Barbara De la Salle

UK NEQAS (H), PO Box 14, WATFORD WD18 0FJ, UK

email: haem@ukneqas.org.uk Phone: + 44 (0)1923 217878

Authorised by: Yvonne John (Service Manager)

© Copyright Notice: UK NEQAS reports are confidential, and no data may be published without the Organiser's permission

Your instrument :

### Your reported results

#### 2101CM1

Sample Quality

Overall :Satisfactory : 98.21% **You reported : Satisfactory**  
Unsatisfactory : 1.79%

Parameter	Result	Trimmed Mean	DI	N	N trimmed	CV%	Uncertainty of target value
Hb (g/L)		190	2.08	56	50		0.002
PCV/Hct (L/L)		0.589	-0.96	56	50		0.006

Reference method results **Hb(g/L)** 200 ( ICSH) **PCV/Hct(L/L)** not available ( Microhaematocrit Centrifuge )

#### 2101CM2

Sample Quality

Overall :Satisfactory : 98.21% **You reported : Satisfactory**  
Unsatisfactory : 1.79%

Parameter	Result	Trimmed Mean	DI	N	N trimmed	CV%	Uncertainty of target value
Hb (g/L)		199	1.46	56	50		0.002
PCV/Hct (L/L)		0.613	-1.52	56	50		0.006

Reference method results **Hb(g/L)** 212 ( ICSH) **PCV/Hct(L/L)** not available ( Microhaematocrit Centrifuge )

#### 2101CM3

Sample Quality

Overall :Satisfactory : 98.21% **You reported : Satisfactory**  
Unsatisfactory : 1.79%

Parameter	Result	Trimmed Mean	DI	N	N trimmed	CV%	Uncertainty of target value
PLT (x10 <sup>9</sup> /L)		1280	-0.41	56	50		0.01

Reference method results **PLT(x10<sup>9</sup>/L)** 1397 ( Immunoplatelet reference method )

#### 2101CM4

Sample Quality

Overall :Satisfactory : 98.21% **You reported : Satisfactory**  
Unsatisfactory : 1.79%

Parameter	Result	Trimmed Mean	DI	N	N trimmed	CV%	Uncertainty of target value
PLT (x10 <sup>9</sup> /L)		1092	-0.15	56	50		0.011

Reference method results **PLT(x10<sup>9</sup>/L)** 1332 ( Immunoplatelet reference method )

Printed at 9:25 on Thursday, 17 June, 2021 (Final Report)

For information on data analysis and performance assessment see the [UK NEQAS Haematology Participant's Manual](#)

Scheme Director: Barbara De la Salle

UK NEQAS (H), PO Box 14, WATFORD WD18 0FJ, UK

email: haem@ukneqas.org.uk Phone: + 44 (0)1923 217878

Authorised by: Yvonne John (Service Manager)

© Copyright Notice: UK NEQAS reports are confidential, and no data may be published without the Organiser's permission